

Importance of Anatoxin-a Determination

Anatoxin-a is an alkaloid neurotoxin produced by some species of cyanobacteria (blue-green algae). It is one of the most toxic of the cyanobacterial toxins. In humans and other animals, the skeletal neuromuscular junction constitutes a primary target for Anatoxin-a (Anatoxin-a can also cross the blood-brain barrier). The neuromuscular junction is specialized for the rapid transmission of neuronal information from the pre-synaptic nerve terminal to the post-synaptic muscle fiber. This transmission is mediated by the synchronous release of the neurotransmitter acetylcholine (ACh), which activates nicotinic acetylcholine receptors (nAChRs) in the muscle endplate, triggering a series of events that lead to muscle contraction. Most ACh molecules are hydrolyzed by acetylcholinesterases, which are highly concentrated at the neuromuscular junction. Anatoxin-a functions as an agonist of nAChRs, like ACh, but is about 20 times more potent. Unlike ACh, it is not degraded by acetylcholinesterases and produces sustained depolarization of the muscle endplate, causing overstimulation of the muscles, leading to muscle fatigue and ultimately paralysis. Symptoms begin within 5 minutes of ingestion of Anatoxin-a and progress rapidly, resulting in cyanosis, convulsions, cardiac arrhythmia, and respiratory paralysis, which ultimately results in death due to suffocation.

Humans and other animals may be exposed to Anatoxin-a through ingestion of contaminated water, through drinking or during recreational activities in which water is swallowed. Due to the potential for serious harm and even death, many countries are expanding monitoring programs to include Anatoxin-a and are establishing regulations regarding the amount of Anatoxin-a in drinking and recreational waters. New Zealand is among those taking regulatory action, establishing a 6.0 µg/L provisional maximum acceptable value (MAV) for Anatoxin-a.

The Abraxis Anatoxin-a Receptor-Binding Assay can be performed in approximately 3.5 hours. Only a few milliliters of sample are required.

Performance Data


Test sensitivity:

The limit of detection for Anatoxin-a is 10 ng/mL. The concentration of residue necessary to cause 50% inhibition (50% B/B₀) is approximately 82.1 ng/mL. Determinations closer to the middle of the calibration range of the test yield the most accurate results.

The assay range is 10 ng/mL to 500 ng/mL. Sample concentration may be performed for samples requiring a lower limit of detection (0.2 ng/mL to 10 ng/mL range). SPE column purchasing information and sample concentration technical bulletin are available from Abraxis by request.

Test reproducibility:

Coefficients of variation (CVs) for standards: <10%; for samples: <15% (based on absorbance).

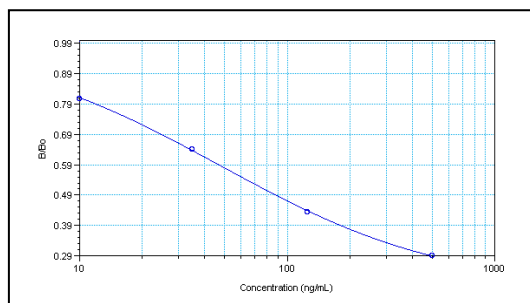

For demonstration purposes only. Not for use in sample interpretation.

References:

**"Procédé de fabrication d'un support d'analyse et utilisation pour la détection des toxines,"* French priority patent application No. 1150586, January 25, 2011 and International patent application No. FR2012050157, January 24, 2012. Licensed exclusively by Abraxis.

General Limited Warranty:

Abraxis, Inc. warrants the products manufactured by the Company against defects and workmanship when used in accordance with the applicable instructions for a period not to extend beyond the product's printed expiration date. **Abraxis makes no other warranty, expressed or implied. There is no warranty of merchantability or fitness for a particular purpose.**

For ordering or technical assistance contact:

Abraxis, Inc.
124 Railroad Drive
Warminster, PA 18974
Tel.: (215) 357-3911
Fax: (215) 357-5232
Email: info@abraxiskits.com
WEB: www.abraxiskits.com

R051017

Anatoxin-a Receptor-Binding Assay* (Microtiter Plate)



Receptor-Binding Assay for the Determination
of Anatoxin-a in Fresh Water

Product No. 520050

1. General Description

The Abraxis Anatoxin-a Receptor-Binding Assay is a patented* receptor-binding assay for the detection of Anatoxin-a in fresh water samples. This test is suitable for the quantitative and/or qualitative detection of Anatoxin-a. Positive samples should be confirmed by HPLC/MS, GC/MS, or other conventional methods.

2. Safety Instructions

The standard solutions in this test kit contain small amounts of Anatoxin-a. In addition, the substrate solution contains tetramethylbenzidine and the stop solution contains diluted sulfuric acid. Avoid contact of these solutions with skin and mucous membranes. If these reagents come in contact with skin, wash thoroughly with water.

3. Storage and Stability

The Anatoxin-a Receptor-Binding Assay Kit should be stored in the refrigerator (4–8°C). The solutions must be allowed to reach room temperature (20–25°C) before use. Reagents may be used until the expiration date on the box.

4. Test Principle

The test is a receptor-binding assay based on the affinity of Anatoxin-a for nicotinic acetylcholine receptors (nAChRs). Anatoxin-a, when present in a sample, will compete with the biotinylated alpha-bungarotoxin for the acetylcholine binding sites of nAChRs, from purified *Torpedo* electrocyte membranes, which were coated on the microtiter plate. After a washing step, a streptavidin-HRP solution is added to allow for the colorimetric detection of the biotinylated alpha-bungarotoxin bound on the receptor. After a second washing step, the substrate solution is added and a color signal is produced. The intensity of the blue color is inversely proportional to the concentration of Anatoxin-a present in the sample. The color reaction is stopped after a specified time and the color (yellow) is evaluated using a microplate photometer. The concentrations of the samples are determined by interpolation using the standard curve constructed with each run.

5. Limitations of the Anatoxin-a Receptor-Binding Assay, Possible Test Interference

Numerous organic and inorganic compounds commonly found in samples have been tested and found not to interfere with this test. However, due to the high variability of compounds that might be found in environmental samples, test interferences caused by matrix effects cannot be completely excluded.

Anatoxin-a will degrade when exposed to natural and artificial light and/or high pH conditions. Samples which have been exposed to natural or artificial light and/or preserved with reagents which raise the natural sample pH may produce results which are biased low. See Section C, Sample Collection and Handling, for appropriate sample handling information.

Mistakes in handling the test can also cause errors. Possible sources for such errors can include:

a) inadequate storage conditions of the test kit, b) incorrect pipetting sequence or inaccurate volumes of the reagents, c) too long or too short incubation times, and d) inadequate temperatures during incubations (<35°C or >40°C during Standard/Sample, Biotinylated Alpha-Bungarotoxin, and Streptavidin incubations and <20°C or >25°C during Color incubation).

The Abraxis Anatoxin-a Receptor-Binding Assay kit provides screening results. As with any analytical technique (GC, HPLC, etc.), positive samples requiring regulatory action should be confirmed by an alternative method.

A. Materials Provided

1. Nicotinic Acetylcholine Receptor (nAChR) coated microtiter plate, 12 strips of 8 wells in a re-sealable pouch
2. Anatoxin-a Standards (5): 0, 10, 35, 125, and 500 ng/mL (ppb), 1 mL each
3. 10X Concentrated Sample Preservation Solution, 25 mL
4. Biotinylated Alpha-Bungarotoxin Solution, 6 mL
5. Streptavidin-HRP Conjugate Solution, 16 mL
6. Sample Diluent, 30 mL
7. Wash Buffer (5X) Concentrate, 100 mL, must be diluted before use, see Test Preparation (Section C)
8. Substrate (Color) Solution (TMB), 16 mL
9. Stop Solution, 12 mL
10. Adhesive Film Plate Cover

B. Additional Materials (not included with the test kit)

1. Micro-pipettes with disposable plastic tips (20-200 μ L)
2. Multi-channel pipette or stepper pipette (50-250 μ L) with disposable plastic tips
3. Deionized or distilled water
4. Graduated cylinder
5. Container with 500 mL capacity (for diluted 1X Wash Buffer, see Test Preparation, Section C)
6. Timer
7. Paper towels or equivalent absorbent material
8. Incubator capable of maintaining 37°C
9. Microtiter plate reader (wave length 450 nm)

C. Sample Collection and Handling

Collect water samples in amber glass sample containers. Immediately upon collection, fresh water samples **must** be preserved using the 10X Sample Preservation Solution (1 mL of 10X Sample Preservation Solution per 9 mL of water sample), to prevent degradation of Anatoxin-a, which will produce inaccurate (biased low) sample results. Drinking water samples should also be treated with ascorbic acid (up to 1 mg/mL) immediately after collection to remove residual chlorine. *Do not use sodium thiosulfate. Sodium thiosulfate will degrade Anatoxin-a and produce biased low sample results.* Store samples refrigerated (4-8°C) for up to 28 days. Samples which must be held for more than 28 days should be stored frozen. Samples should be protected from exposure to natural and artificial light, as light exposure will cause degradation of Anatoxin-a. Do not preserve samples with reagents which will raise the natural sample pH. If sample pH must be adjusted for extraction or concentration purposes, brief exposure to high pH conditions will not adversely affect results, but prolonged exposure to high pH conditions should be avoided.

If total Anatoxin-a concentration (free and cell-bound) is required, an appropriate cell lysing procedure (freeze and thaw, sonication, QuikLyse™, etc.) must be performed prior to analysis.

If large amounts of organic matter are present, samples may be filtered prior to analysis (PALL Life Sciences Acrodisc® 25 mm Syringe Filters (PALL part number 4612) are recommended). If determining total Anatoxin-a concentration, samples should be lysed prior to filtration to prevent the removal of cell-bound Anatoxin-a, which would cause inaccurate results.

D. Test Preparation

Micro-pipetting equipment and pipette tips for pipetting the standards and samples are necessary. A multi-channel pipette or a stepping pipette is recommended for adding the Biotinylated Alpha-Bungarotoxin, Streptavidin-HRP Conjugate, substrate (color), and stop solutions in order to equalize the incubations periods of the solutions on the entire microtiter plate. Please use only the reagents and standards from one package lot in one test, as they have been adjusted in combination.

1. Allow the microtiter plate, reagents, and samples to reach room temperature before beginning the test.
2. The microtiter plate consists of 12 strips of 8 wells. The recommended run size is 6 strips or less, as drift may occur. Use of more than 6 strips in an analytical run may cause inaccurate results. Analysis in **triplicate** is highly recommended.
3. Remove the number of microtiter plate strips required from the foil bag. The remaining strips must be stored in the foil bag with desiccant and zip-locked closed. Store the remaining kit in the refrigerator (4-8°C).
4. The standard solutions, sample diluent, Biotinylated Alpha-Bungarotoxin, Streptavidin-HRP, substrate (color), and stop solutions are ready to use and do not require any further dilutions.
5. Dilute the Wash Buffer (5X) Concentrate at a ratio of 1:5 with deionized or distilled water. If using the entire bottle (100 mL), add to 400 mL of deionized or distilled water.
6. The stop solution must be handled with care as it contains diluted H₂SO₄.
7. The adhesive film plate cover should be used to cover the wells during the incubation periods. Wells should be sealed closed to prevent evaporative loss. The cover can be used for multiple runs; do not discard the backing – replace on the adhesive portion of the cover after each use.

E. Working Scheme

The microtiter plate consists of 12 strips of 8 wells, which can be used individually for the test. The recommended run size is 6 strips or less, as drift may occur. Use of more than 6 strips in an analytical run may cause inaccurate results. Analysis in **triplicate** is highly recommended. The standards must be run with each test. Never use the values of standards which have been determined in a test performed previously.

	1	2	3	4	5	6	7	8	9	10	11	12
A	Std 0	Std 2	Samp 1									
B	Std 0	Std 3	Samp 1									
C	Std 0	Std 3	Samp 2									
D	Std 1	Std 3	Samp 2									
E	Std 1	Std 4	Samp 2									
F	Std 1	Std 4	etc.									
G	Std 2	Std 4	etc.									
H	Std 2	Samp 1	etc.									

Std 0-Std 4: Standards

0; 10; 35; 125; 500 ppb

Samp 1, Samp 2, etc.: Samples

F. Assay Procedure

1. Add **100 μ L of the standard solutions and preserved freshwater samples** into the wells of the test strips according to the working scheme given. Analysis in **triplicate** is recommended. Cover the wells with the adhesive film plate cover and mix the contents by moving the strip holder in a circular motion on the benchtop for 60 seconds. Be careful not to spill the contents. Incubate the strips in an incubator at 37°C for 2 hours.
2. Remove the covering and add **50 μ L of biotinylated alpha-bungarotoxin solution** to the individual wells successively using a multi-channel pipette or a stepping pipette. Cover the wells with the adhesive film plate cover and mix the contents by moving the strip holder in a circular motion on the benchtop for 60 seconds. Be careful not to spill the contents. Incubate in an incubator at 37°C for 30 minutes.
3. Remove the covering and vigorously shake the contents of the wells into a sink. Wash the strips **three times** using the diluted wash buffer. Use at least a volume of **250 μ L of 1X wash buffer** for each well and each washing step. Remaining buffer in the wells should be removed by patting the inverted plate dry on a stack of paper towels.
4. Add **150 μ L of streptavidin-HRP conjugate solution** to the individual wells successively using a multi-channel pipette or a stepping pipette. Cover the wells with the adhesive film plate cover and mix the contents by moving the strip holder in a circular motion on the benchtop for 60 seconds. Be careful not to spill the contents. Incubate in an incubator at 37°C for 30 minutes.
5. Remove the covering and vigorously shake the contents of the wells into a sink. Wash the strips **three times** using the diluted wash buffer. Use at least a volume of **250 μ L of 1X wash buffer** for each well and each washing step. Remaining buffer in the wells should be removed by patting the inverted plate dry on a stack of paper towels.
6. Add **150 μ L of substrate (color) solution** to the wells using a multi-channel pipette or a stepping pipette. Cover the wells with the adhesive film plate cover and mix the contents by moving the strip holder in a circular motion on the benchtop for 60 seconds. Incubate for 30 minutes at **room temperature**. Protect the strips from direct sunlight.
7. Add **100 μ L of stop solution** to the wells using a multi-channel pipette or a stepping pipette in the same sequence as for the substrate solution.
8. Read the absorbance at 450 nm using a microplate ELISA photometer within 15 minutes after the addition of the stopping solution.

G. Evaluation

The evaluation of the assay can be performed using commercial ELISA evaluation programs (4-Parameter (preferred) or Logit/Log). For manual evaluation, calculate the mean absorbance value for each of the standards (B_i). Calculate the %B_i/B₀ for each standard by dividing the mean absorbance value for each standard by the Zero Standard (Standard 0) mean absorbance (B₀). Construct a standard curve by plotting the %B_i/B₀ for each standard on the vertical linear (y) axis versus the corresponding Anatoxin-a concentration on the horizontal logarithmic (x) axis on graph paper. %B_i/B₀ for samples will then yield levels in ppb of Anatoxin-a by interpolation using the standard curve; results for preserved water samples are determined by multiplying the concentration determined by the curve by the dilution factor of 1.1. Samples showing lower concentrations of Anatoxin-a compared to Standard 1 (10 ng/mL) should be reported as containing < 11 ng/mL of Anatoxin-a. Samples showing a higher concentration than Standard 4 (500 ng/mL) should be reported as containing > 550 ng/mL of Anatoxin-a. If a quantitative result is necessary, samples must be diluted further and re-analyzed to obtain accurate results.